

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

SEP 17 2009

DataMaster cdm S/N: <u>130113</u>	
Supervisor/Operator Performing the Verification Procedure:	
Name: <u>Kenneth G. Cox</u>	ID #: <u>3527</u> Date: <u>September 14, 2009</u>
A Agency: <u>Skagway Police Department</u>	Phone #: <u>907 983-2232</u>
Instrument Location <u>Skagway Police Department, 1<sup>st</sup> &amp; State Street Skagway, Alaska 99840</u>	
Alco S/N <u>X173010</u>	Target Value <u>.082</u> High Pressure <u>400</u>
Alco Test Value Average <u>.081</u>	<u>.081</u>
1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco
Signature <u><i>Kenneth G. Cox</i></u>	
(OVER)	

(Do Not write in the area below)

*BMB*  
*9/22/09*

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

*Nita J. Bolz*  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this \_\_\_\_\_ day of \_\_\_\_\_, 2009.

(Notary Seal Stamp)

Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

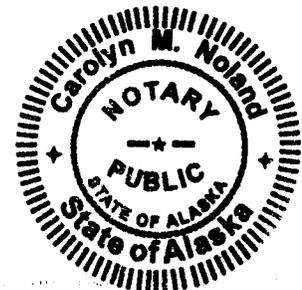

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130113

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130113

SEPTEMBER 14, 2009

OPERATOR'S NAME: *SMB 9/22/09*  
COX/KENNETH/G  
OPERATOR'S NUMBER: 3527  
SUBJECT'S LAST NAME:  
VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI :

L  
O.L. #: L  
DEPT/AGENCY: SK61  
CASE/REPORT: 2009

ALCO TARGET VALUE: .082  
ALCO S/N: K173010

— BREATH ANALYSIS —

.082 ADJUSTED FOR 30.11 in		
ALCO TARGET	.082	09:43
BLANK TEST	.000	09:44
INTERNAL STANDARD	VERIFIED	09:44
ALCO TV 30.11 in	.081	09:45
BLANK TEST	.000	09:46
SUBJECT SAMPLE	.000	09:46
BLANK TEST	.000	09:47
ALCO TV 30.11 in	.081	09:48
BLANK TEST	.000	09:49

*SMB 9/22/09*

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130113

SEPTEMBER 14, 2009  
TIME 09:39

— DIAGNOSTIC CHECK —

COMPUTER: OKAY ✓  
PROGRAM: OKAY ✓  
SOFTWARE DATE: 02/20/01 ✓  
HEATERS  
SAMPLE CHAMBER: 49c ✓  
BREATH TUBE: 41c ✓  
BAROMETER: 30.11 in ✓  
FLOW DETECTOR: OKAY ✓  
PUMP  
HIGH SPEED: OKAY ✓  
DETECTOR: OKAY ✓  
FILTERS: OKAY ✓  
QUARTZ STANDARD: OKAY ✓  
CALIBRATION: OKAY ✓

PRINTER TEST

! " # \$ % & ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z ( ) ~ |